


Auerbach Mallet Splint


600

Warnings and Instructions: Review carefully, proper application is required


⚠ Warning: This device will not prevent or eliminate risk of injury. Do Not Overtighten. If swelling, pain, skin irritation, or an unusual reaction occurs, discontinue use immediately and consult your medical professional. This device should not be worn by persons with known allergies to neoprene. Care: Hand wash using mild soap. Rinse thoroughly. Air dry only. Do not tumble dry.

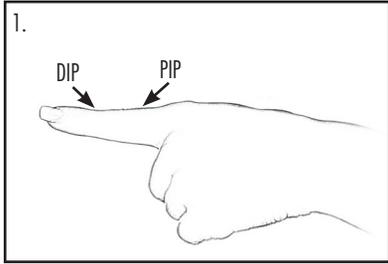


1. The DIP joint must be kept in a straight position at all times. Holding the fingertip on the edge of a counter, place the splint on the nail side of the finger with the rubber surface in contact with the skin.

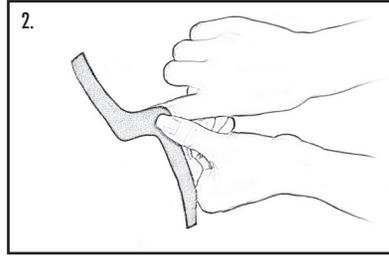


2. Apply the splint with the transverse strap closer to the hand and the angled strap over the nail.

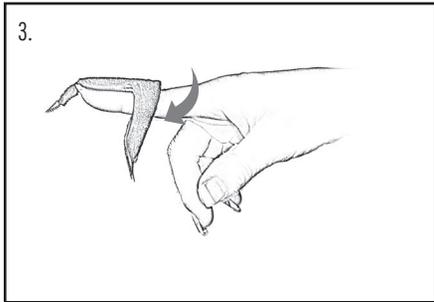

3. Secure the transverse strap.

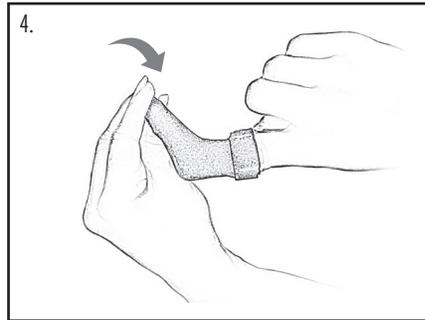

4. Secure the angled strap. The straps should hold the splint firmly, but should not be too tight as to interfere with circulation to the fingertip.

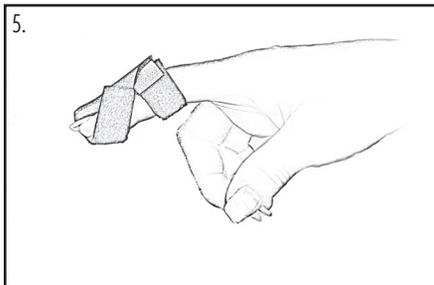

5. Completed application. The PIP joint should move freely.

HELY & WEBER
© 2023 Weber Orthopedics Inc.
DBA Hely & Weber all rights reserved

1185 E Main St., Santa Paula, California 93060
California: 800-221-5465, National: 800-654-3241
International: 805-525-4244, fax: 805-933-2348
U.S. fax: 800-559-5975, www.hely-weber.com

Rev D 04/23

CE


MDSS GmbH, Schiffgraben 41
30175 Hannover, Germany

Auerbach Mallet Splint


600

Warnings and Instructions: Review carefully, proper application is required


⚠ Warning: This device will not prevent or eliminate risk of injury. Do Not Overtighten. If swelling, pain, skin irritation, or an unusual reaction occurs, discontinue use immediately and consult your medical professional. This device should not be worn by persons with known allergies to neoprene. Care: Hand wash using mild soap. Rinse thoroughly. Air dry only. Do not tumble dry.

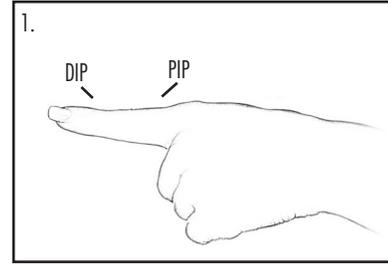


1. The DIP joint must be kept in a straight position at all times. Holding the fingertip on the edge of a counter, place the splint on the nail side of the finger with the rubber surface in contact with the skin.

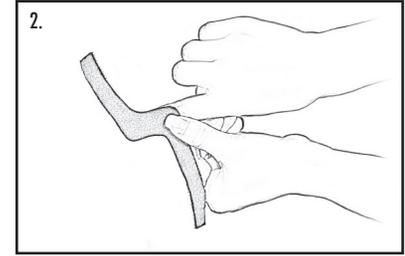


2. Apply the splint with the transverse strap closer to the hand and the angled strap over the nail.

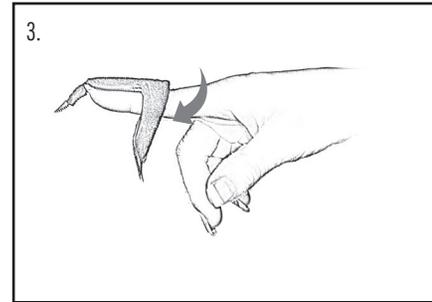

3. Secure the transverse strap.

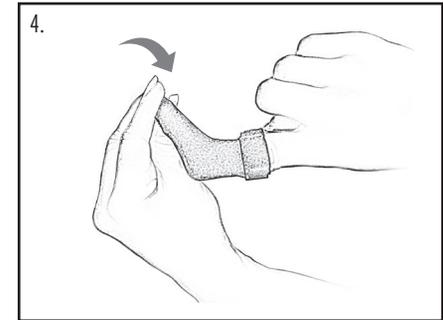

4. Secure the angled strap. The straps should hold the splint firmly, but should not be too tight as to interfere with circulation to the fingertip.

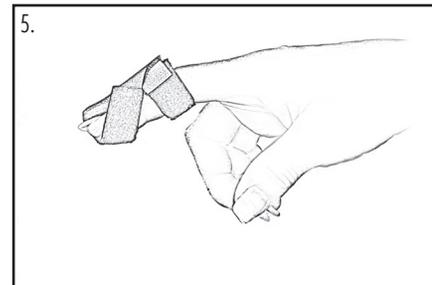

5. Completed application. The PIP joint should move freely.

HELY & WEBER
© 2023 Weber Orthopedics Inc.
DBA Hely & Weber all rights reserved

1185 E Main St., Santa Paula, California 93060
California: 800-221-5465, National: 800-654-3241
International: 805-525-4244, fax: 805-933-2348
U.S. fax: 800-559-5975, www.hely-weber.com

Rev D 04/23

CE

MDSS GmbH, Schiffgraben 41
30175 Hannover, Germany