


**Warnings and Instructions: Review carefully, proper application is required**


**⚠ Warning:** This device will not prevent or eliminate risk of injury. Do Not Overtighten. If swelling, pain, skin irritation, or an unusual reaction occurs, discontinue use immediately and consult your medical professional.

This device should not be worn by persons with known allergies to neoprene.


Care: Hand wash using mild soap. Rinse thoroughly. Air dry only. Do not tumble dry.

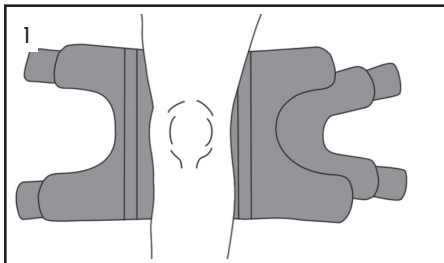


1. Remove buttress from inside of brace. With leg fully extended center brace on leg between stay pockets.

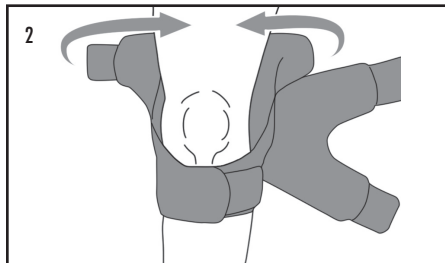


2. Pull and fasten lower and upper straps.

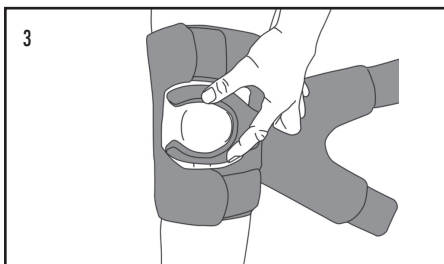

3. Place the buttress with the smooth side down against the kneecap as prescribed by a medical professional.

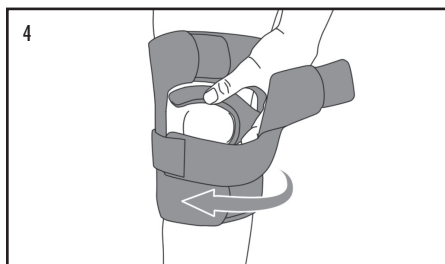

4. While holding the buttress in place, secure the buttress by pulling and fastening the lower and upper flap straps across the buttress.

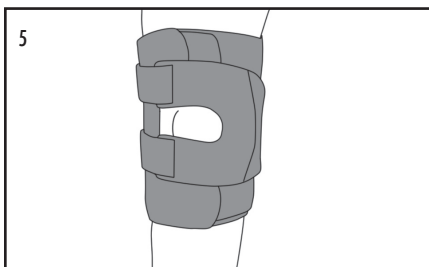

5. Completed application.

U.S. Patent No. 5759167



Scan to watch application video



© 2014 Weber Orthopedics Inc.  
DBA Hely & Weber all rights reserved  
1185 E Main St., Santa Paula, California 93060  
California: 800-221-5465, National: 800-654-3241  
International: 805-525-4244, fax: 805-933-2348  
U.S. fax: 800-559-5975, www.hely-weber.com



MDSS GmbH, Schiffgraben 41  
30175 Hannover, Germany


Rev C 3/14

**Warnings and Instructions: Review carefully, proper application is required**


**⚠ Warning:** This device will not prevent or eliminate risk of injury. Do Not Overtighten. If swelling, pain, skin irritation, or an unusual reaction occurs, discontinue use immediately and consult your medical professional.

This device should not be worn by persons with known allergies to neoprene.


Care: Hand wash using mild soap. Rinse thoroughly. Air dry only. Do not tumble dry.

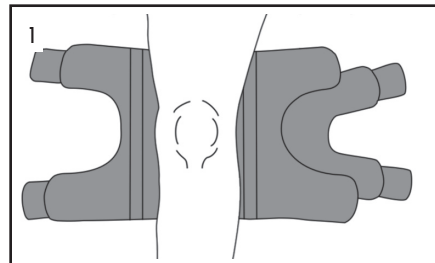


1. Remove buttress from inside of brace. With leg fully extended center brace on leg between stay pockets.

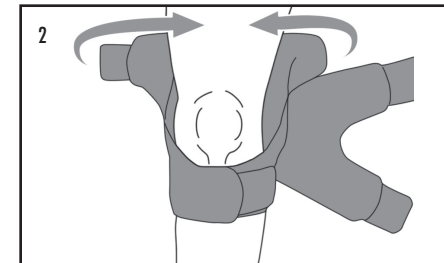


2. Pull and fasten lower and upper straps.

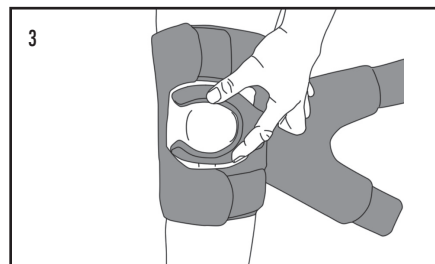

3. Place the buttress with the smooth side down against the kneecap as prescribed by a medical professional.

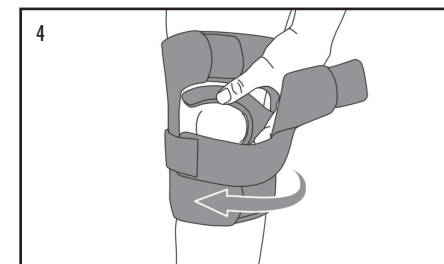

4. While holding the buttress in place, secure the buttress by pulling and fastening the lower and upper flap straps across the buttress.

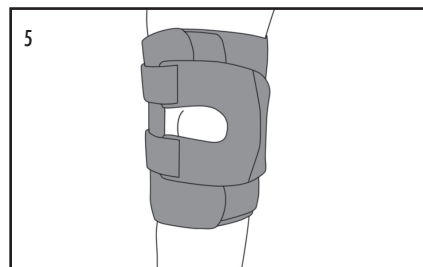

5. Completed application.

U.S. Patent No. 5759167



Scan to watch application video



© 2014 Weber Orthopedics Inc.  
DBA Hely & Weber all rights reserved  
1185 E Main St., Santa Paula, California 93060  
California: 800-221-5465, National: 800-654-3241  
International: 805-525-4244, fax: 805-933-2348  
U.S. fax: 800-559-5975, www.hely-weber.com



MDSS GmbH, Schiffgraben 41  
30175 Hannover, Germany

Rev C 3/14