


# TINY POST-OP KNEE

**Warnings and Instructions: Review carefully, proper application is required** 220


**⚠ Warning:** This device will not prevent or eliminate risk of injury. Do Not Overtighten. If swelling, pain, skin irritation, or an unusual reaction occurs, discontinue use immediately and consult your medical professional.

This device should not be worn by persons with known allergies to neoprene.


Care: Hand wash using mild soap. Rinse thoroughly. Air dry only. Do not tumble dry.

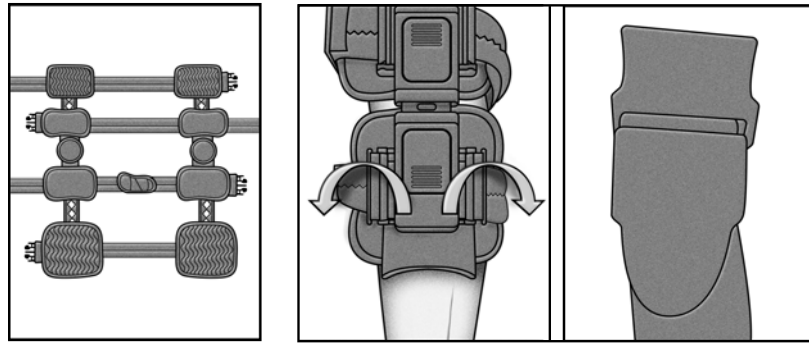


1. Unbuckle straps and lay brace flat.
2. Open strap locks on each of the four sliders with the receiving end of the buckle for size adjustments.

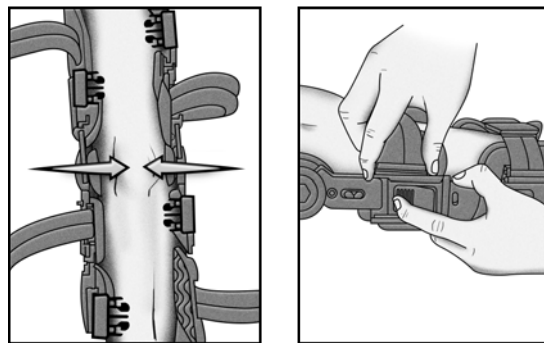

3. Slide brace onto leg with shorter upright applied to the thigh. Center the uprights directly medial and lateral and the hinge on joint center.
4. Depress ribbed area on side button to telescope sliders. First, for length, adjust most proximal and distal slider and second, for strap position, the two inner sliders.

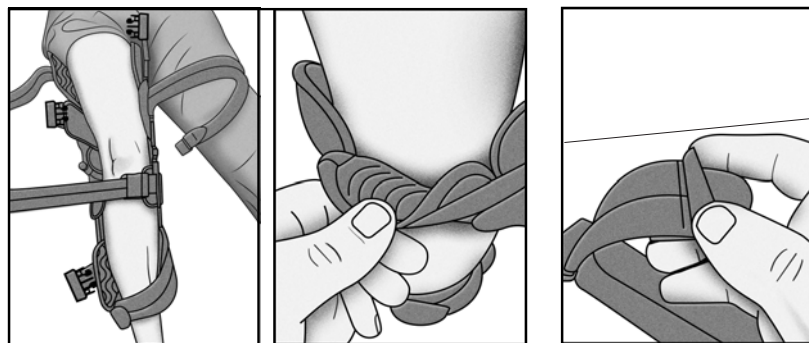

5. Click male end of buckle into female end and tighten strap 1 just distal from center knee. Position silicone pad on back of strap so it rests on top of the calf.
6. Cut padded strap length so it attaches to itself posteriorly and reposition the alligator clip at end of cut strap to secure.

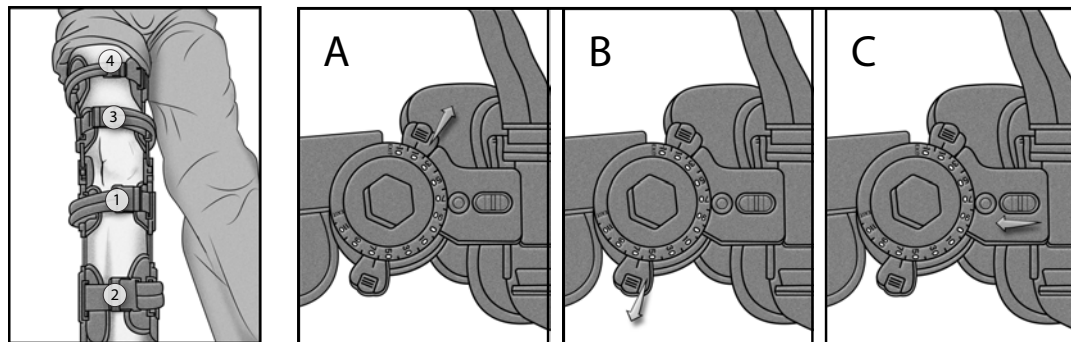

7. Repeat steps 5 and 6 on each strap in sequence shown above.
8. Set Flexion (A) and extension (B) to degrees desired by lifting up tamper pin and slide stop to appropriate degrees. For drop lock, push up slide to lock (C).



1185 E Main St., Santa Paula, California 93060  
California: 800-221-5465, National: 800-654-3241  
International: 805-525-4244, fax: 805-933-2348  
U.S. fax: 800-559-5975, www.hely-weber.com

Rev D 8/24




# TINY POST-OP KNEE

**Warnings and Instructions: Review carefully, proper application is required** 220


**⚠ Warning:** This device will not prevent or eliminate risk of injury. Do Not Overtighten. If swelling, pain, skin irritation, or an unusual reaction occurs, discontinue use immediately and consult your medical professional.

This device should not be worn by persons with known allergies to neoprene.


Care: Hand wash using mild soap. Rinse thoroughly. Air dry only. Do not tumble dry.

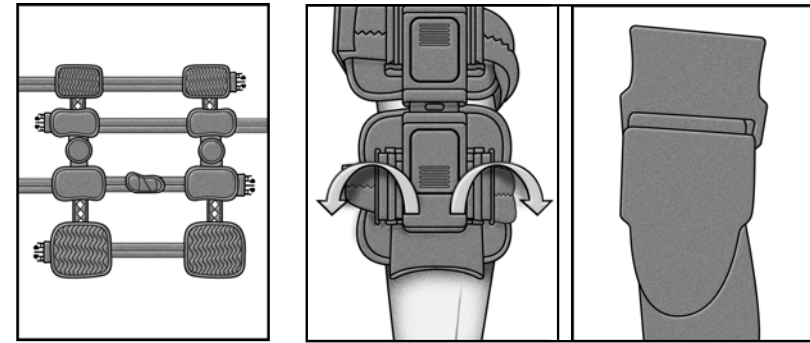


1. Unbuckle straps and lay brace flat.
2. Open strap locks on each of the four sliders with the receiving end of the buckle for size adjustments.

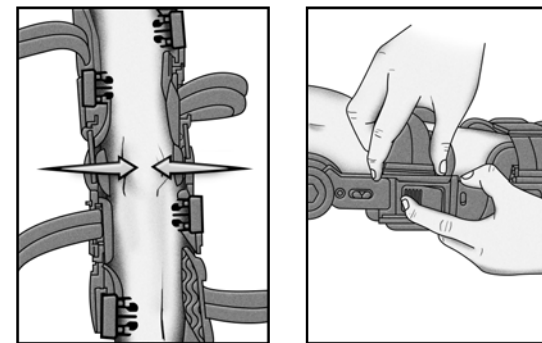

3. Slide brace onto leg with shorter upright applied to the thigh. Center the uprights directly medial and lateral and the hinge on joint center.
4. Depress ribbed area on side button to telescope sliders. First, for length, adjust most proximal and distal slider and second, for strap position, the two inner sliders.

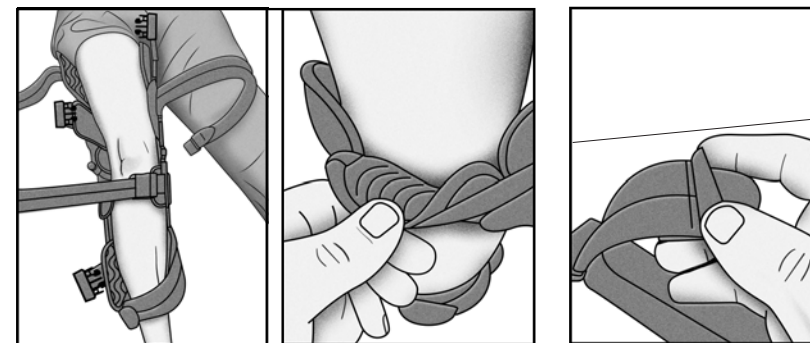

5. Click male end of buckle into female end and tighten strap 1 just distal from center knee. Position silicone pad on back of strap so it rests on top of the calf.
6. Cut padded strap length so it attaches to itself posteriorly and reposition the alligator clip at end of cut strap to secure.

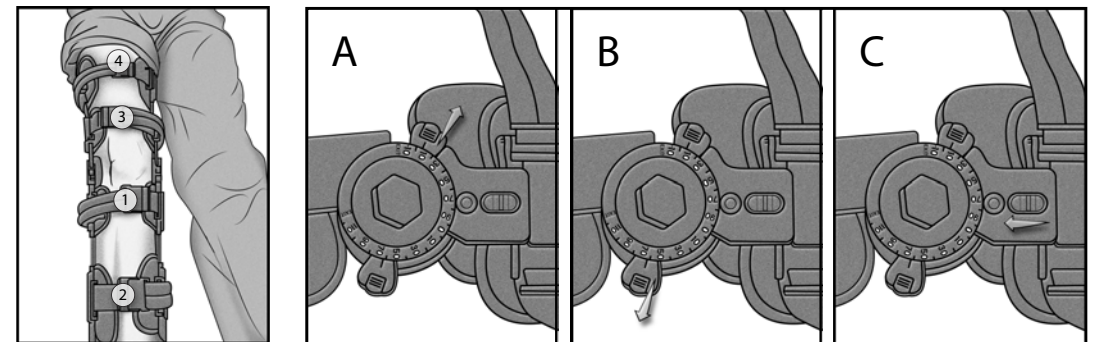

7. Repeat steps 5 and 6 on each strap in sequence shown above.
8. Set Flexion (A) and extension (B) to degrees desired by lifting up tamper pin and slide stop to appropriate degrees. For drop lock, push up slide to lock (C).



1185 E Main St., Santa Paula, California 93060  
California: 800-221-5465, National: 800-654-3241  
International: 805-525-4244, fax: 805-933-2348  
U.S. fax: 800-559-5975, www.hely-weber.com

Rev D 8/24

