


**Warnings and Instructions: Review carefully, proper application is required**


**⚠ Warning:** This device will not prevent or eliminate risk of injury. Do Not Overtighten. If swelling, pain, skin irritation, or an unusual reaction occurs, discontinue use immediately and consult your medical professional.

This device should not be worn by persons with known allergies to neoprene.


Care: Hand wash using mild soap. Rinse thoroughly. Air dry only. Do not tumble dry.

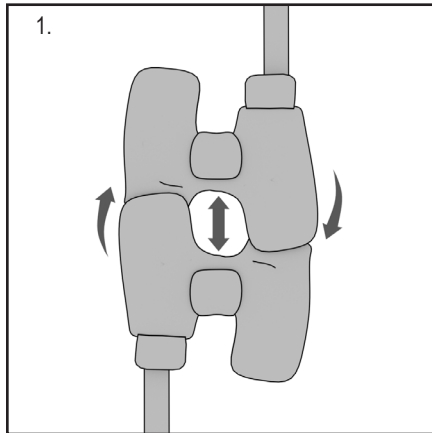


1. Open front brace enclosures. Adjust width of brace so that epicondyles align with condyle pads.

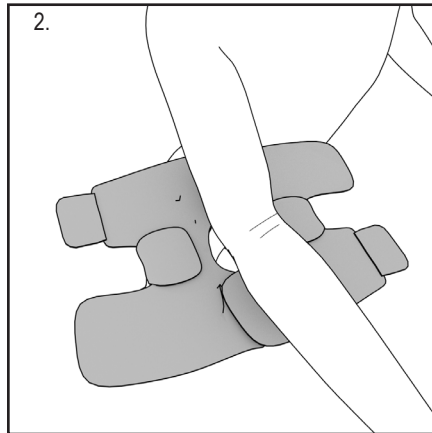


2. Place arm with the cubital fold centered in brace.

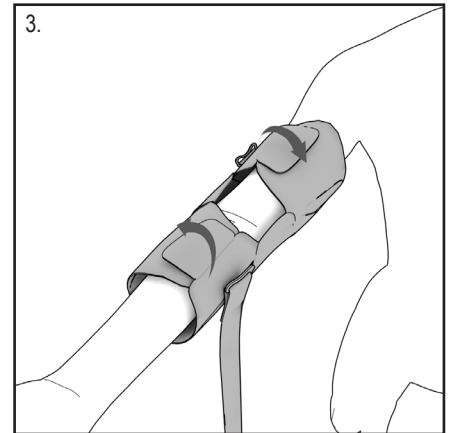

3. Pull and fasten elbow flaps.

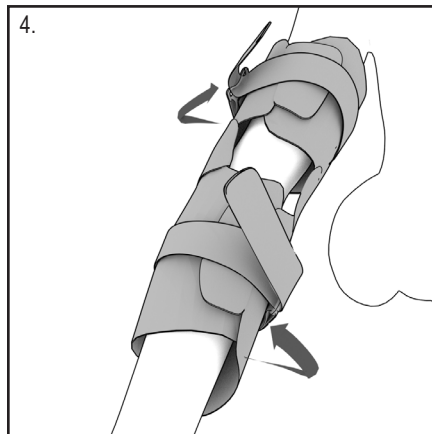


4. Fasten D-ring straps.

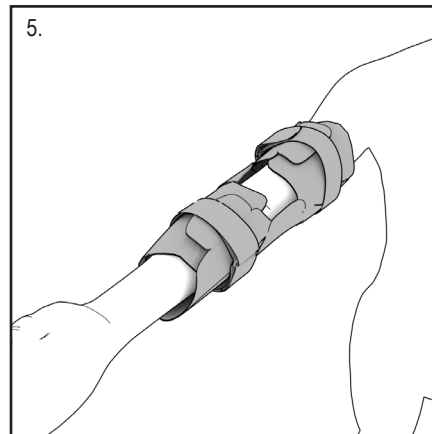


5. Finished application.


**ADJUSTING THE HINGE RANGE OF MOTION**

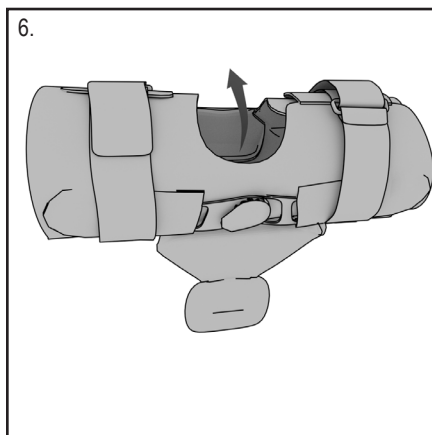

6. Remove brace and open condyle hinge cover to expose hinges.

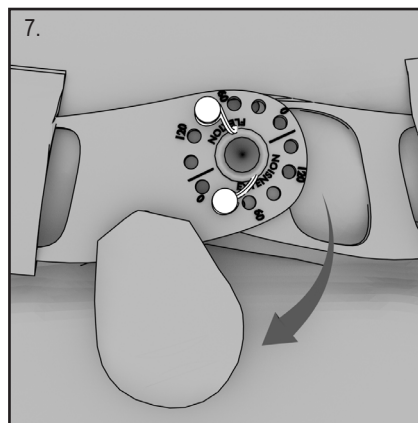

7. Rotate open hinge stop cover, and adjust hinge stop pins for desired range of motion. Both medial and lateral hinges must be set to the same setting. Close hinge stop cover.

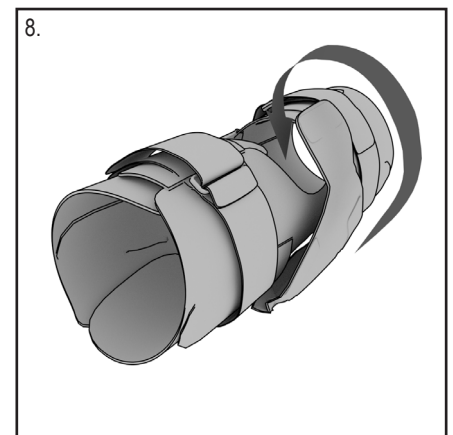

8. Re-attach condyle hinge cover.



Scan for video